

# Medical Emergency Assistance System using GSM

B. Jyosthna<sup>1</sup>, R. GiriPrasad<sup>2</sup>

<sup>1</sup>M.Tech Student, Dept. of ECE, Prakasam Engineering College, Kandukur, Prakasam (DT), A.P, India

<sup>2</sup>Associate professor, Dept. of ECE, Prakasam Engineering College, Kandukur, Prakasam (DT), A.P, India

**Abstract:** *Medical Emergency Assistance System is continues monitoring system of health conditions and send the information regularly to the hospital. Care of critically ill patient, requires spontaneous & accurate decisions so that life-protecting & lifesaving therapy can be properly applied. Medical Emergency system is realized as an embedded device. The concept is implemented in the emulator with GSM real hardware interface. Communication between Hospital and the device is by GSM technology. I have designed and developed a reliable, energy efficient remote patient monitoring system. It enables the doctors to monitor patient's parameters (temp, heartbeat, ECG) in real time through an SMS.*

**Keywords:** Sensors, ARM 7 microprocessor, GSM modem

## 1. Introduction

In the field of health monitoring the current most important user groups are those aged 40 and more. The group of 40+ users shows more diversity in their health conditions than younger people. There are ring-type pulses monitoring sensor available in the market in which the measured data are displayed in the LCD and cannot be transmitted out of the ring. Thus, it is not possible to continuously monitor the vital parameters such as temperature, pressure and pulse from a distant location. In a hospital either the nurse or the doctor has to move physically from one person to another for health check, which may not be possible to monitor their conditions continuously. Thus any critical situations cannot be found easily unless the nurse or doctor checks the person's health at that moment. This may be a strain for the doctors who have to take care of a lot number of people in the hospital.

In order to keep in track of critical health conditions, a real time health monitoring system of patient based on GSM, and SMS is designed and developed in this project. This finds vast application in the remote places where the people are out of reach from the experienced doctors; keeping this factor in mind best effort is done to implement some of the basic test of pathological data on the system. Hence the entire project can be broadly divided into four sections firstly, the parameters measured from the patient and transmitted, secondly the signal processing and conversion to digital form; thirdly decision making with the help of an algorithm where they obtained signal values are compared with the standard values and finally the transmission of the condition of the patient to the doctor.

A real time health monitoring system of remote patient developed is a wearable device. This device will be wearied by the patient and parameters such as ECG, Temperature and Heart Beat will be continuously transmitted and monitor through wireless technology GSM. At the receiver side (doctor side) the data will be wirelessly received using GSM. The doctor will monitor

the measured parameter on the GUI designed using Visual Basic on PC. The data from the patient is collected continuously and stored in the database designed using SQL (Structured Query Language) if the doctor is not present at that instant of time, he will be intimated through an SMS (Short Messaging Service)also the relatives will receive a message in case of abnormalities . On detecting the type of abnormality the doctor can call the patient and let him know the further course of action.

## 2. Problem Statement

There are some shortcomings present in existing system. Currently there are number of health monitoring systems available for the ICU patients which can be used only when the patient is on bed. This system is wired everywhere. The patient is monitored in ICU and the data transferred to the PC is wired. Such systems become difficult where the distance between System and PC is more. The available systems are huge in size. Regular monitoring of patient is not possible once he/she is discharged from hospitals. These systems cannot be used at individual level.

The other problem with these systems is that it is not capable of transmitting data continuously also range limitations of different wireless technologies used in the systems. So to overcome these limitations of systems I have proposed a new system. This system is able to transmit the parameters of patient continuously and over long distance wirelessly. Due to which we would be able attend the patient immediately. Therefore by developing a system that can constantly measure the important parameters of patient's body and which can alert the closed ones and the doctor on any time when the patient's condition gets bad, this can really provide quick service and be beneficial in saving a lot of lives.

## 3. Proposed System

The system which we proposed to develop shown in figure.2 would not only help in monitoring the patient when he is in the bed but also when he is not in the bed

i.e. when he is mobile. Such a system would constantly monitor important body parameters like temperature, heartbeat, ECG and would compare it against a predetermined value set and if these values cross a particular limit it would automatically alert the doctor and relatives of the patient via a SMS. In such case the patient will get a very quick medical help and also would save time and energy of the relatives who would not be with them all the time.

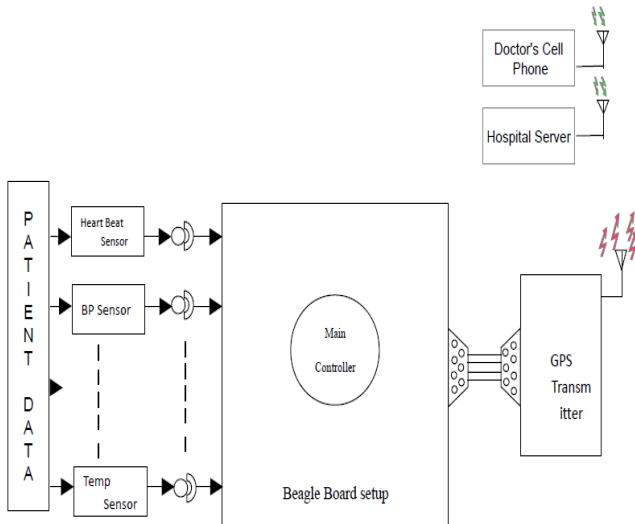


Figure 1: Proposed Systems

This system provides a continuous health monitoring service for patient. Temperature, ECG and Heart Beat pulse signals are measured from the temperature, ECG and heart beat sensors and are processed by a built-in ARM processor. The processed data are then transmitted by GSM wirelessly. Finally the received data is sent to the PC. The graphical user interface programs on the PC are coded using Visual Basic language. In the PC a coding is written using Visual basic for transmitting the information of any abnormal health conditions to the specified mobile number (of the doctor in charge) in the program through a GSM modem. Embedded C is used for programming the ARM processor. Using GSM modem message is transmitted to the programmed mobile number to the doctor in charge when the measured temperature exceeds the allowable value or if the pulse measured is abnormal.

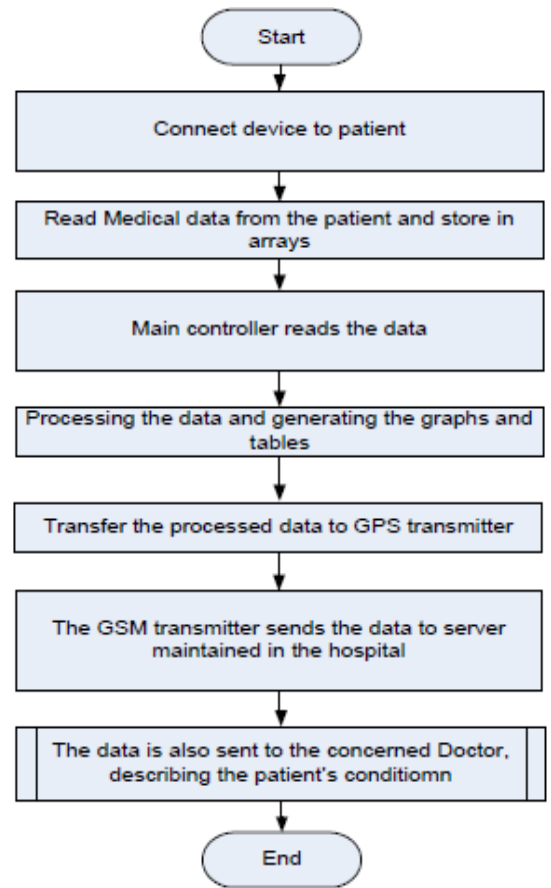


Figure 2: Flow chart of the proposed System

## 4. Designing

The designing part includes basically three sections as follows;

### 4.1 Hardware Design

It includes Power supply design, Temperature sensor, Heart beat sensor, ECG sensor, ARM processor and GSM connector circuit.

- GSM modules shall be connected via serial port.
- Serial port has to connect to the emulator/ Real board.
- Emulator/Board shall communicate to the GSM module through serial.
- GSM modules have to be prepared with valid SIM card and power supply.
- HARDWARE : SIM 300 MODULES
- COMMUNICATION : RS232
- COMMANDS: AT Commands shall be used to communicate with GSM module Refer SIM300 AT Command Set.

#### 4.1.1 Power Supply Circuit

Hardware requires different power supplies.

- 5 v: for temperature sensor circuit, heartbeat circuit, RS 232 connector circuit
- 12v: for ARM 7processor.
- +/- 9v: for ECG sensor circuit

#### 4.1.2 ARM 7Processor

The ARM7 is a general purpose 32-bit microprocessor, offers high performance and very low power consumption. ARM architecture is based on RISC principles, instruction set and related decode mechanism are simpler than CISC Pipeline techniques employed ARM Processor supports both 32-bit and 16-bit instructions via the ARM and Thumb instruction sets. The 3 parameters to be monitored are sensed using respective sensor and data is feed to ARM7 .Traditionally, embedded devices include two types of processors: a Microcontroller and a DSP to process signals. However, with the development of ARM processors, last two can be replaced by one single processor. This unit is the heart of the complete system. It is actually responsible for all the process being executed. It will monitor & control all the peripheral devices or components connected in the system. In short we can say that the complete intelligence of the project resides in the software code embedded in the ARM 7. The code will be written in Embedded C and will be burned or programmed into the code memory using a programmer.

#### 4.1.3 ECG Sensor

ECG is primarily a tool for examination of cardiac diseases. An ECG sensing device commonly consists of a group of electrodes to detect electrical events of a heart. The ECG is the electrical manifestation of the contractile activity of the heart, and can be recorded fairly easily with surface electrodes on the limbs or chest. The rhythm of the heart in terms of beats per minute (bpm) may be easily estimated by counting the readily identifiable waves. The amplifier takes the input from 3 electrodes which are connected to the patient.

#### 4.1.4 Temperature Sensor LM35

LM35 series are precision integration-circuit temperature sensors whose output voltage is linearly proportional to the Celsius temperature. The LM35 does not require any external calibration or trimming to provide typical accuracies. This is 3 legs IC that directly gives analog output. This unit requires +5VDC for it proper operation.

#### 4.1.5 Heart Beat Sensor

Heart beat sensor is designed to give digital output of heart beat when a finger is placed inside it. This digital output can be connected to ARM directly to measure the Beats per Minute (BPM) rate. It works on the principle of light modulation by blood flow through finger at each pulse. ICLM358is used for Heart Beat Sensor. Its dual low power operational amplifier consists of a super bright red LED and light detector. One will act as amplifiers and

another will be used as comparator. LED needs to be super bright as the light must pass through finger and detected at other end. When heart pumps a pulse of blood through blood vessels, finger becomes slightly more opaque so less light reached at the detector. With each heart pulse detector signal varies this variation is converted to electrical pulse.

GSM (Global System for Mobile communications)

GSM (Global System for Mobile communications) is an open, digital cellular technology used for transmitting mobile voice and data services.GSM supports voice calls and data transfer speeds of up to 9.6 kbps, together with the transmission of SMS (Short Message Service).

GSM can be operated from any distance to any point of control. The communication is done with the help of local network support. This can get communicated to any part of the world which the network of the local system is applicable. Here we are using for the hospital communication for monitoring the patient.

#### 4.2 Software Design

- 1) Main task will provide the graphics display of different sensor inputs.
- 2) It shall provide the interface to send "location request messages" from GSM module.
- 3) Software modules have to do the serial communication implementation compatible with GSM hardware module.
- 4) GSM module related commands have to be selected depend on the sensor data.
- 5) During software implementation on emulator the data will be simulated for minimum, medium and extreme conditions.
- 6) Communication protocols:

The data has to be send to GSM module from emulator by serial communication. The specifications for serial communication are:

- Baud rate = 9600 bauds
- Transfer packet length= 8 bits
- Parity = no parity
- Hard ware control = None
- Mode = Bidirectional

### 4.3 User Interface Requirement

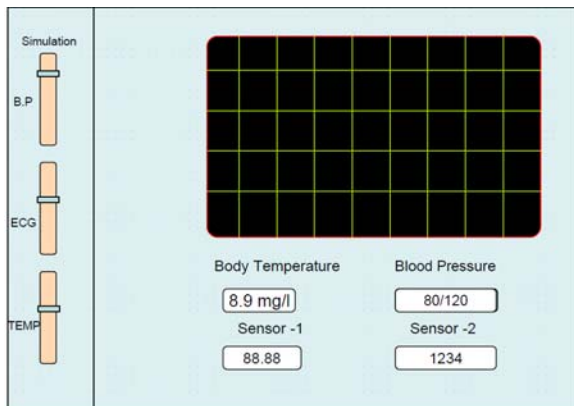


Figure 3: User Interface Requirement

### 5. Conclusion

From the above designed project we are able to transmit the data which is sensed from remote patient to the server PC by using wireless transmission technology GSM. Using GSM at receiver the data is received and displayed on the PC of doctor. Also if doctor is not present in campuses he will receive SMS on his mobile phone in case any parameter of the goes beyond the normal range. The leads of the ECG sensor must be stick properly to the patient, which is nearest to the chest side of patient. So that we get more and more correct ECG.

### References

- [1] 'International Cardiovascular Disease Statistics, Statistical Fact Sheet-2007 Update', American Heart Association, Dallas, Texas, 2007
- [2] Lai Khin Wee, Yeo Kee Jiar, Eko Supriyanto "Electrocardiogram Data Capturing System and Computerized Digitization using Image Processing Techniques" International Journal of Biology and Biomedical Engineering Issue 3, Volume 3, 2009
- [3] Khoór S, Nieberl J, Fügedi K, Kail E 'Internet based, GPRS, long term ECG monitoring and nonlinear heart-rate analysis for cardiovascular telemedicine management' Computers in Cardiology 2003;28:209-212.
- [4] Ljupčco Hadžievski, Boško Bojovic, Vladan Vukčević, Petar Beličev, Siniša Pavlovic, Zorana Vasiljevic-Pokrajčic, and Miodrag Ostojic "A Novel Mobile Transtelephonic System With Synthesized 12-Lead ECG" IEEE Transaction on Information Technology in Biomedicine, Volume 8, 2004
- [5] Dr.R.Sukanesh, S.Palanivel rajan, S.Vijayprasath, S.Janardhana prabhu and P.Subathra 'gsm based ecg tele-alert system', Department of Electronics and Communication Engineering, Dept. of Electron. & Commun. Eng., Thiagarajar Coll. of Eng., Madurai, India Innovative Computing Technologies (ICT), International Conference 2010

- [6] Sukanesh.R; Gautham.P; Rajan S.P ; Arunmozhivarman P.T ; Vijayprasath S. 'Cellular phone based biomedical system for health care' Dept. of Electron. & Commun. Eng., Thiagarajar coll. of Eng., Madurai, India Communication Control and Computing Technologies (ICCCCT), IEEE International Conference 2010
- [7] V.Ramya, B.Palaniappan, Anuradha Kumari 'Embedded Patient Monitoring System' International Journal of Embedded Systems and Applications (IJESA) Vol.1, No.2, December 2011
- [8] Prof. Dr. Burkhard Stiller 'Mobile Healthcare on Android Devices' Communication Systems Group, Diploma Thesis, Dept. of Informatics, November 2010
- [9] Alma Secerbegovic, Aljo Mujčić, Nermin Suljanović, Midhat Nurkic, Jurij Tasic 'The research mHealth platform for ECG monitoring', ConTel Conference, 2011

### Author Profile

**B. Jyosthna** received B.TECH degree in Electronics and Communications Engineering Prakasam Engineering College from JNTU University, Hyderabad, in 2007. He is currently doing M. Tech in Prakasam Engineering College, from JNTUK University, Kakinada. His research interests include VLSI and Embedded systems.

**R. GiriPrasad** received B.E, M.Tech degree. Working as an Associate professor for Dept. of ECE in Prakasam Engineering College, Kandukur, Prakasam (DT), A.P, India.