

Study of Heating Process in Condenser of Thermokinetic Desorptor

Shital Dharmul¹, D. S. S. Sudhakar²

¹M.E (Mechanical-CAD/CAM & ROBOTICS) Production Engineering Department, Fr. Conceicao Rodrigues College of Engineering Bandra Mumbai University, Mumbai, Maharashtra, India

²Professor, Production Engineering Department, Fr. Conceicao Rodrigues College of Engineering Bandra Mumbai University, Mumbai, Maharashtra, India

Abstract: *Volatile is a substance which can change state from a solid or liquid to vapor. Gas chromatography (GC) is the instrument used to study volatiles and it can analyse molecules whose boiling points are as high as 250°C or more. Thermokinetic Desorptor is a sampling device for GC which doesn't allow non volatile material in GC column. Condenser plays a vital role in separating volatiles from nonvolatile material. The aim of current study to analyses heating process in condenser to get optimum temperature while separating volatiles.*

Keywords: Desorptor Cartridge Heaters, Temperature, Ambient Temperature, Conductive Heat Transfer, Specific Heat.

1. Introduction

The report describes study of new approach of heating process in MATLAB environment. PDE APP MATLAB tool is used to analyse heating process. The Prototype device for this is already manufactured, which is a POC (Proof of Concept). The goal of this report is to reduce the time of heating. For the purpose of heating the envelope electrical heaters are used with sensor for establishment of feedback control system peltier chips are used for cooling process.

A method of analysis and the associated MATLAB software results are presented for the purpose of solving steady and transient state nonlinear heat transfer problem in condenser. Nonlinearity arises due to dependence of thermal conductivities on temperature as well as from presence of radioactive heat transfer.

2. Literature Review

Following literature describes the prototype thermokinetic desorptor developed previously. This device works on thermo-Kinetic Principle of extraction. The equipment contains following parts [4]:

1. PID Controller.
2. Electrical Circuit.
3. Flow and Temperature control.
4. Desorptor and Condenser.
5. Absorbent.
6. Heating and cooling Media.
7. Critical components of the system are design and geometry of Desorptor and Condenser, selection of heating and cooling media, absorbent material, and feedback control system for governing temperature, flow and Pressure.

2.1 Description of various sub-systems:

2.1.1 The Desorptor

Desorptor is a single piece unit carved out of 316 grade stainless steel (food and surgical grade, ideal for pressure reactors and boilers and is corrosion resistant) and fitted with screw cap for sample load. A GC septum or O rings secured airtight sealing. Holes are drilled in the body to accommodate the cartridge type heaters and temperature sensors. The sample compartment is cylindrical with 1 cm diameter and 5 cm length. Special care is taken to polish the interiors to avoid sample retention and subsequent contamination. Ferrule nuts are welded in the body for nitrogen inlet and effluent outlet. The heaters and sensors are connected to the thermostat and can be programmed from ambient temperature to 350°C in multi steps.

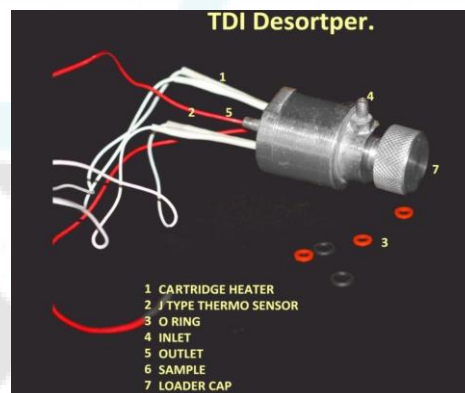


Figure 1: Old model of Desorptor

2.1.2 Condenser

The condenser unit is slightly more complex than the desorptor both in functioning and in construction. The main body is 316 stainless steel cylinders with a 1cm x 6cm hole drilled in. The adsorbent material is packed in here. It has inlet and outlet holes fitted with ferrule nuts. Glass wool protects these holes from adsorbent choking. A special heater with inbuilt thermo sensors is wound around

the condenser tightly. This heater is capable of heating the condenser to $250^{\circ}\text{C} \pm 1^{\circ}\text{C}$ in just 5 seconds, and maintains the temperature so. The temperature range and holding time can be programmed. An Aluminium sleeve perfectly fits around the heating element, giving it a close contact with cooling system outside. The cooling system consists of two aluminium boxes with cylindrical slit at its centre. These boxes are driven with a lever system to separate them from the condenser or to bring them close to the aluminium sleeve. The coolant used is a mixture of dry ice and acetone.

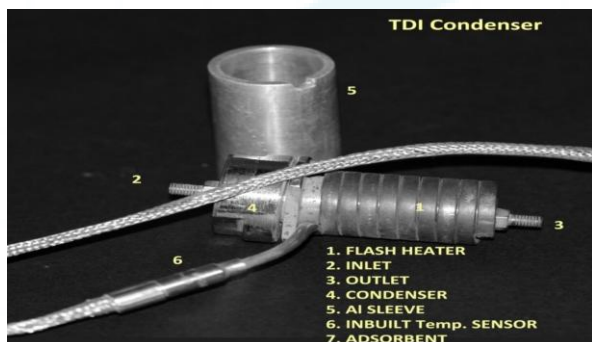


Figure 2: Old model of Condenser

2.2. Working

A solid or semisolid sample containing volatiles is heated using multiple sources in a current of dry or moist (Controlled) Nitrogen and the effluents are driven to a frigid cartridge pre-loaded with appropriate adsorbent. Once the desorption is complete, the cartridge can be flash heated and the pneumatics drive the volatiles through appropriate membrane filters to the GC for analysis. Membrane filters are used to selectively detain water molecules and molecules of particular choice.

3. Method

The function of condenser is to concentrate the volatiles by first cooling them up to -30°C and trapping it with in absorber. Absorber is a porous material which only allows nitrogen gas to pass through and will trap volatile. Again to release the volatiles absorber is flash heated up to 250°C . Then it delivers the volatile in GC machine. Fig 2 shows the view of previous condenser and porous adsorbent material. We modified the design of component.

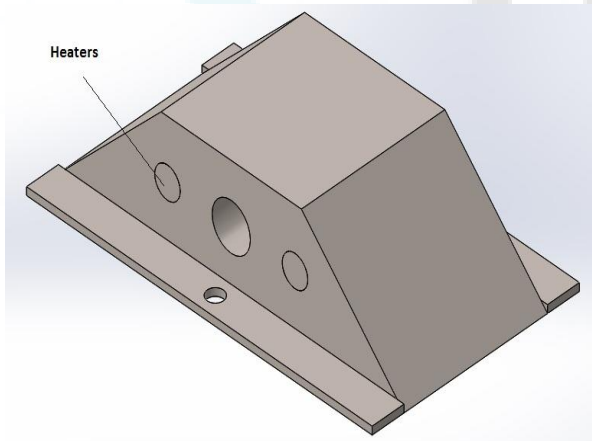


Figure 3: New modified condenser model

Figure above shows the condenser model with two cartridge heaters. Following boundary condition was applied:

Initial Temperature – 20°C

Maximum Temperature – 250°C

Heat Transferred from heaters to Condenser:

$$Q = m c_p (t_2 - t_1) = 80.5 \text{ KW}$$

Where,

m = Mass of Condenser Body

c_p = Specific heat of stainless steel

Time of heating = 300 seconds

3.1 Heating Process

After cooling process, the volatiles are trapped in the absorber porous material. Further these volatiles need to be released from the porous zone. In order to release them, we need to heat the condenser up to temperature 250°C in 5 minutes. For heating purpose it is decided to use cartridge heaters for ease of manufacturing & operation. Special bore for accommodation were provided as shown Figure 3.

Wattage calculation for Cartridge heaters:

$$W = \frac{\text{Wt.} \cdot C_p \cdot \Delta T}{3412 \cdot H} = 471.86 \text{ watts} = 500 \text{ watts}$$

$W = 500 \text{ Watt}$

Wt = weight of material to be heated = 0.7 kg

C_p = Specific Heat of Stainless steel = $500 \text{ J/kg}^{\circ}\text{K}$

ΔT = Temperature rise = 230°C

H = Heating time in Hours = 0.05

By calculation, It is decided to use 2 heaters of 250 watts.

Specification of Heaters:

Size – $\varnothing 8 \times 31 \text{ mm}$

Sensor – PT 100

4. Mathematical Modeling

The partial differential equation of heat transfer in linear case is:

$$\rho C_p \frac{\partial T}{\partial t} - \nabla \cdot (k \nabla T) = Q \quad (1)$$

T is the temperature, ρ is the material density, C_p is the specific heat, and k is the thermal conductivity. Q is the heat generated. But in nonlinear condition both radiation and convection heat loss considered

Heat transfer is:

$$\rho C_p \frac{\partial T}{\partial t} - (\nabla k \nabla T) + 3hcT + 3\varepsilon\sigma T^4 = 3hcT_a + 3\varepsilon\sigma T_a^4 \quad (2)$$

Where, the factors of three account for the heat transfer from three condenser faces. And T_a is a ambient temperature 300k,

The amount of heat transferred from each face per unit area due to convection is defined as:

$$Q_c = hc(T - T_a) \quad (3)$$

The amount of heat transferred from each face per unit area due to radiation is defined as:

$$Q_r = \epsilon\sigma(T^4 - T_a^4) \quad (4)$$

5. Result

Partial Differential Equation Toolbox provides functions for solving partial differential equations (PDEs) in 2-D, 3-D, and time using finite element analysis. It specifies mesh 2-D and 3-D geometries and formulates boundary conditions and equations.

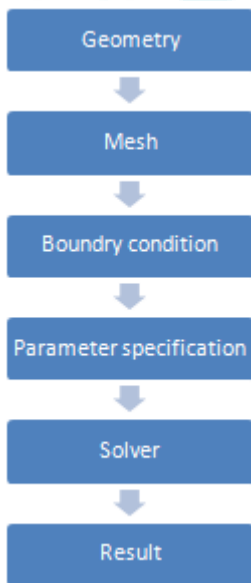


Figure 4: Process Diagram Of PDE App

CONDENSER With Triangular Element Mesh)

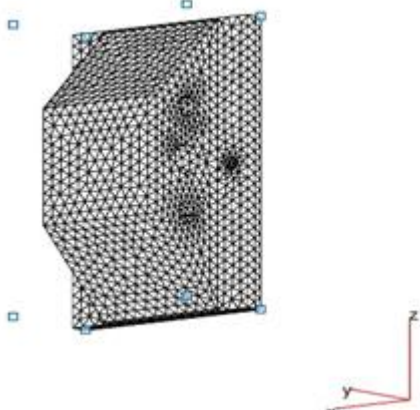


Figure 5: condenser with triangular element mesh

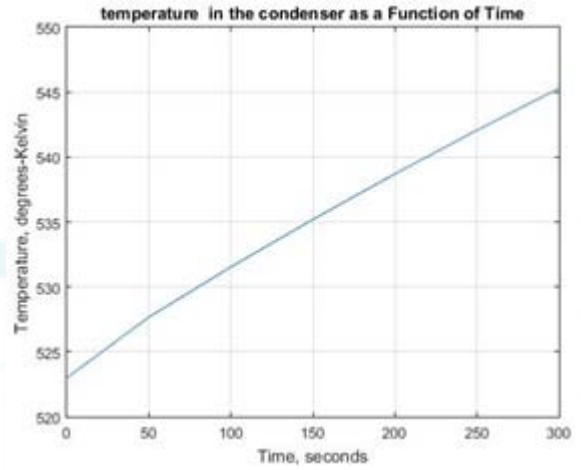


Figure 6: Graph of Temperature Vs. Time for Condenser

Figure: 6 show the relation between time and temperature rise. So the graph shows that after 100 seconds the temperature of condenser reaches near 523k.and after 300sec it reaches to548k.

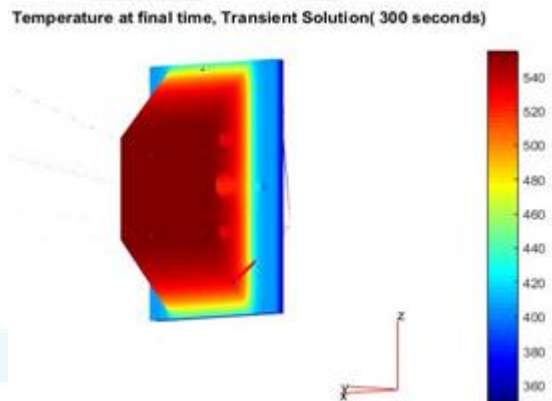


Figure: 7Temperature contour for condenser

Figure: 7 shows temperature contour for condenser. The temperature 523k is given to the heaters and analysis shows that the complete unit will heat up near 548k in 5 minutes. The radiation, conduction, convection losses are considered.

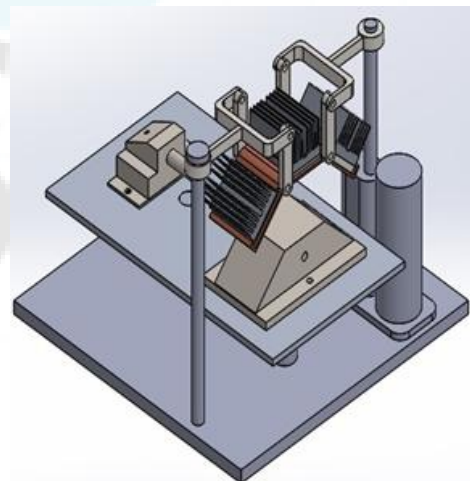


Figure 8: CAD Model of Thermokinetic desorpter Assembly with Condenser

6. Conclusion

After analyzing heating process in MATLAB environment, it is observed that overall condenser effectively heated within minimum temperature.

In the future scope, the volatile separating mechanism can be further developed by improving some factors like heating sources and more efficient peltier chips. Heating sources like Induction, magnetic, microwave and laser heating may have different results, depending on nature sample to be used in order desorbs out more molecules.

References

- [1] B.S.Ajit Kumar, Ajit Datar, "Designing and Construction of a Volatile Separating and Sampling Device Based on Thermo Kinetic Principles" Gurunanak Khalsa college, Mumbai, 2013.)
- [2] Dr. R. Yadav, "Heat and Mass Transfer", Central Publishing House, Allahabad, 2007, pp 177-224.
- [3] Prasad Kawade, Ajit Kumar, Kashyap Anandpara, D.S.S.Sudhakar "Computer Aided Design And Analysis Of Volatile Separating Device" Proceedings of 4th International Conference on Advances in Computing, Communication and Control (ICAC3'15) Volume49, 2015, pages 356-370
- [4] D.Roncati, "Iterative calculation of the heat transfer coefficient", Progettazione Ottica Roncati, Italy, 2013.
- [5] Samet.Y. Kadioglu, Robert R.Nourgaliev, Vincent A.Moussau, "A Comparative Study of the Harmonic and Arithmetic Averaging of Diffusion Coefficients for Non-linear Heat Conduction Problems" INL/EXT-08-13999, 2008-03-01, Idaho National Laboratory (INL) United States
- [6] PDE App MATLAB Tool Documentation

Author Profile



Shital Dharmul Received The Graduation Degree in Mechanical Engineering from Government College of Engineering, Amaravati, Maharashtra In 2011. She is currently pursuing Master of Engineering from. Fr. Conceicao Rodrigues College of Engineering Bandra Mumbai University, She Worked as a Lecturer in Fr. Conceicao Rodrigues College of Engineering Bandra.